
# Soft Tissue Neck W+WO IV Contrast Protocol


Revised: 05/11/22
Charge as: Soft Tissue W+WO IV Contrast
Scanner: 1.5T or 3T
Coil: Head Coil + Neck Coil or Flex Coil (Neck Coil or Flex Coil may be required on certain systems)

| Plane | Weighting | Slice | Gap | FAT SAT | Scan Range |
|---|---|---|---|---|---|
| **COR** | T1 | 4mm | .8mm | None | Nose tip-spinous process/Frontal Sinus-Clavicle/parallel to cervical spine |
| **COR** | STIR | 4mm | .8mm | None | Nose tip-spinous process/Frontal Sinus-Clavicle/parallel to cervical spine |
| **AXIAL** | T1 | 4mm | .8mm | None | Frontal Sinus-Clavicle/perpendicular to cervical spine |
| **AXIAL** | T2 FS | 4mm | 1mm | Strong | Frontal Sinus-Clavicle/perpendicular to cervical spine |
| **SAG** | T1 | 4mm | 1mm | None | Rt to Lt pinna/Frontal Sinus-Clavicle/parallel to cervical spine |
| **AXIAL** | Diffusion | 4mm | 0mm | None | Frontal Sinus-Clavicle/perpendicular to cervical spine |
| **Inject Contrast** | | | | | |
| **COR** | T1 FS | 4mm | 1mm | Strong | Nose tip-spinous process/Frontal Sinus-Clavicle/parallel to cervical spine |
| **AXIAL** | T1 FS | 4mm | 1mm | Strong | Frontal Sinus-Clavicle/perpendicular to cervical spine |
| **SAG** | T1 FS | 4mm | 1mm | Strong | Rt to Lt pinna/Frontal Sinus-Clavicle/parallel to cervical spine |

## COR Soft Tissue Neck Image Planning:

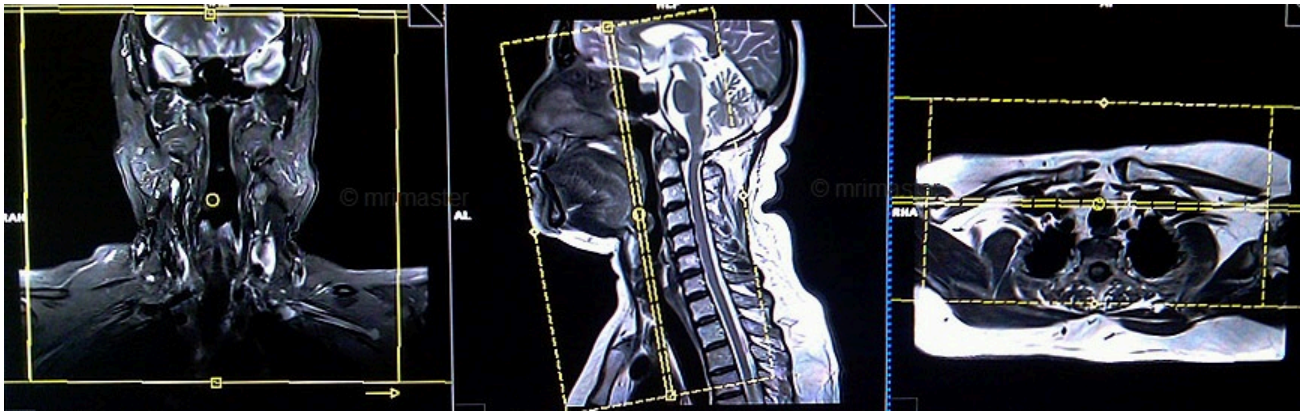

## AXIAL Soft Tissue Neck Image Planning:

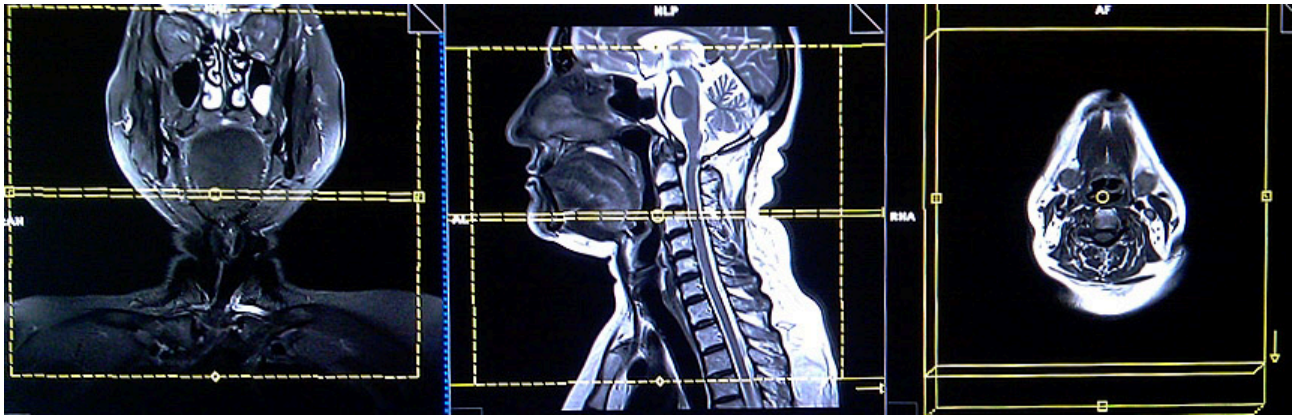

**SAG Soft Tissue Neck Image Planning:**

