


Designing a Flow System for Sustainable Chemistry

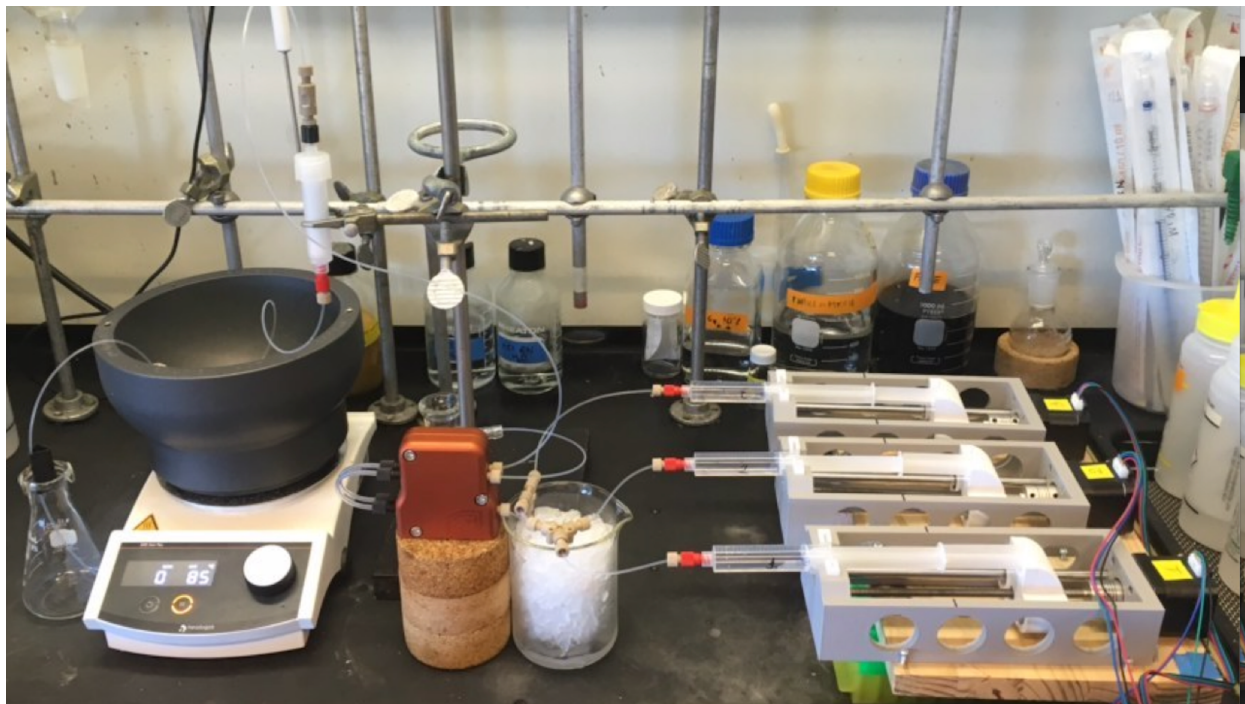

Department of Mechanical and Aerospace Engineering
Mechanical Engineering Program
University of California, San Diego
Instructor: Dr. Huihui Qi

Sponsor:
Dr. [Haim Weizman](#)
Department of Biochemistry and Chemistry, UCSD

Team 3:
Eden Detmer
Nhat Tang
Shravan Suresh
Zaivy Gonzalez-Valencia

Table of Contents

Abstract.....	XX
Table of Contents.....	XX
List of Figures	XX
List of Tables.....	XX
Chapter 1: Project Description	XX
Background.....	XX
Review of Existing Design Solutions.....	XX
Statement of Requirements.....	XX
Deliverables.....	XX
Chapter 2: Description of Final Design Solution.....	XX
Chapter 3: Design of Key Components.....	XX
Modular Syringe Pump.....	XX
User Interface.....	XX
Electronics Housing.....	XX
Chapter 4: Prototype Performance.....	XX
Performance Metrics.....	XX
Tests and Conditions.....	XX
Results.....	XX
Final Performance Evaluation.....	XX
Chapter 5: Design Recommendations and Conclusions.....	XX
Design Recommendations for Future Modifications.....	XX
Impact on Society.....	XX
Professional Responsibility.....	XX
Conclusions.....	XX
Acknowledgements.....	XX
References	XX
Appendix.....	XX
Project Management.....	XX

Abstract


This project, sponsored by Dr. Haim Weizman of the Department of Chemistry and Biochemistry at UCSD, focuses on the development of a user-friendly, low-cost, and do-it-yourself (DIY) flow system. The sponsor's goal is to design a syringe pump system that is paired with an intuitive user interface to increase the prevalence of flow systems in undergraduate laboratories and to provide students with a positive user experience. To achieve this the main target was that it is cost effective, open source, that is the design and the parts are easily accessible and compatible/easy to set up by a user from any background. The system consists of a syringe pusher actuated by a stepper motor which is controlled by an Arduino and receives input commands from the user. Major requirements for the system include a straightforward user interface, compact housing of the electronics, and a modular syringe pump. The system should be accompanied by a simple assembly and operating instructions manual.

Chapter 1 ; Project Description

Background:

The practice of synthesizing chemicals has relied on low technology equipment such as glass flasks and pipettes for decades. These practices are outdated in a world of modern technology and leave a great deal to be desired in terms of both safety and efficiency. Flow chemistry was invented in order to modernize and advance the practice of synthesizing chemicals. In flow chemistry reactions are conducted continuously as reagents are pumped through tubing and mix to form a product. Figure 1 presents a schematic diagram demonstrating the process of flow chemistry.

Figure 1. Flow chemistry schematic (Zaiput Flow Technologies).

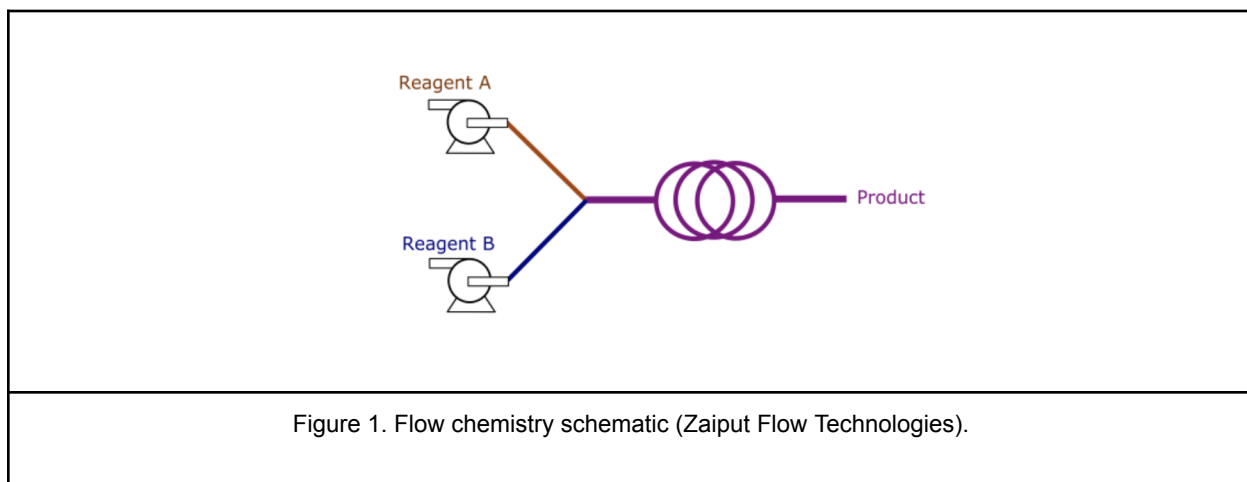

Flow chemistry exhibits numerous benefits over traditional laboratory techniques. Reactions are safer due to the smaller volume of hazardous materials reacting at once, are more efficient due to the high surface area to volume ratio which increases the kinetics of the reactions, and exhibit better control because reactors can be kept at specific temperatures and pressures (Zaiput Flow Technologies). Additionally, flow chemistry is more environmentally friendly and has generated new ways to manufacture sustainable materials. However, one large downside of flow chemistry is its substantial price tag. Commercially available systems cost upwards of \$20,000. Figure 2 displays a \$20,000 chemistry flow system located in the Burkart Laboratory, UCSD. This high price point makes it such that this technology is largely unavailable to academic laboratories and undergraduate students.


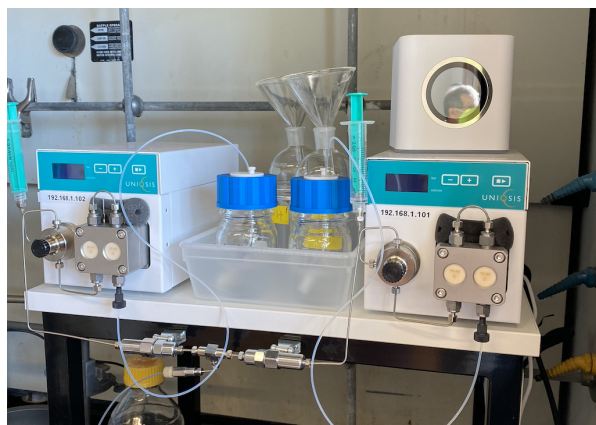


Figure XX. \$20,000 flow chemistry system.

The sponsor of this project, Dr. [Haim Weizman](#), a researcher and professor with the Department of Biochemistry and Chemistry, UCSD, hopes to make a chemistry flow system which is cost-effective and therefore accessible to undergraduate laboratories. With primary research interests of improving organic chemistry instruction at a college level and developing comprehensive laboratories to better train chemistry majors, Dr. Weizman hopes to see new cost-effective and user-friendly flow chemistry systems implemented in undergraduate laboratories in order to educate and inspire chemistry students.

Review of Existing Design Solutions:

Other researchers and professionals have likewise recognised the need for a cost-effective alternative to the costly commercially available flow systems. Therefore, various low-cost, DIY (Do It Yourself) flow chemistry systems have been developed. Namely, the Croatt Research Group at UNC, Greensboro has developed a DIY flow system which is open access and can be manufactured using only a 3D printer and parts ordered from Amazon. This system costs around \$150 total - roughly a 100th of the cost of commercial systems. The system consists of a syringe pump actuated by a stepper motor which is controlled with an Arduino. Figure 3 displays a model of the Croatt Research Group's system.

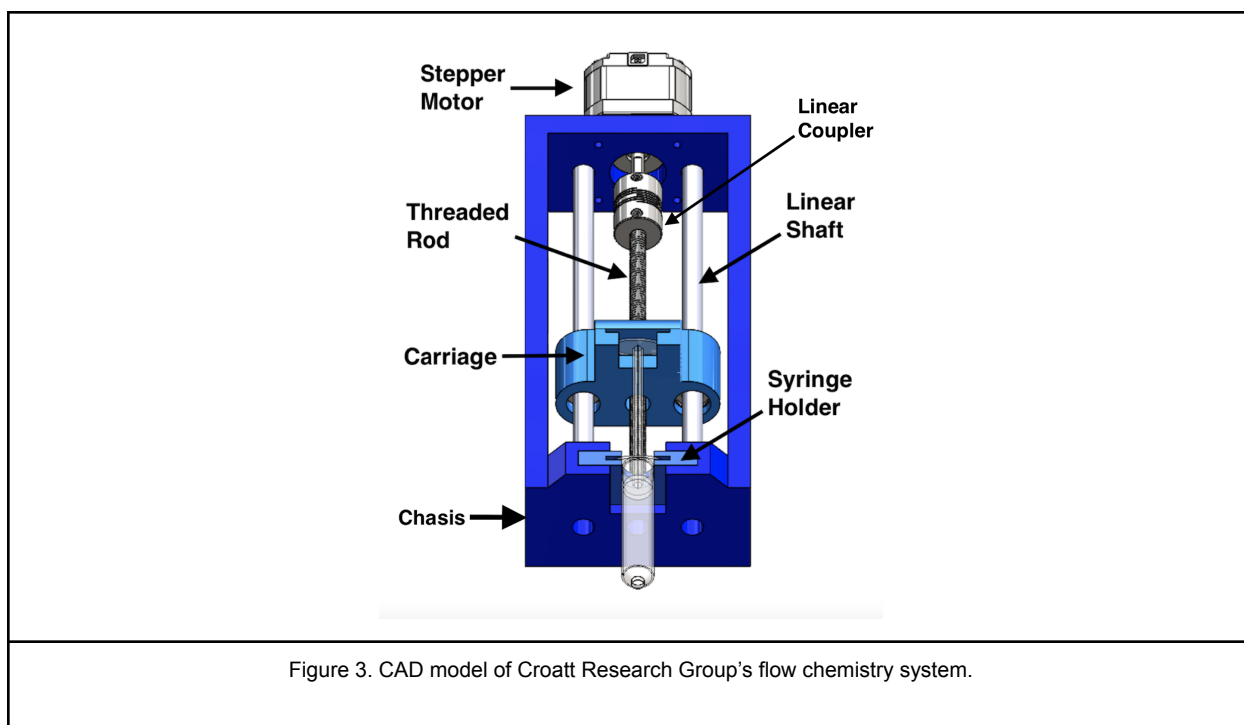

The Croatt Research Group's system functions as a basic flow system, however, the overall user-friendliness of the system leaves something to be desired. A laptop must be connected to the Arduino in order to control the system. Since space is highly limited in many laboratories, having a laptop connected to the system poses an inconvenience. Additionally, the user input commands to the serial monitor on the laptop are not intuitive, especially considering that many chemistry students have limited experience with coding. Furthermore, the Croatt Research Group's system offers little in terms of wire management. As can be seen in Figure 4, many wires are needed to connect the components of the system, resulting in a large nest of wires. Having exposed and mismanaged wires is inconvenient and unsafe to have in a chemistry laboratory. Another issue with the system is that the steel threaded rod experiences corrosion after being left in the fume hood while reactions take place. The system fits syringes of size 1,3,5, and 10 mL. The syringe holder is specific to the size of syringe being used, so multiple differently sized syringe holders are required, along with steps to exchange them when a different syringe is used.

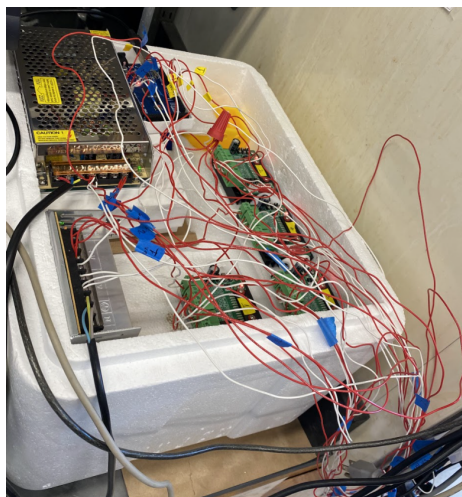


Figure 4. Arduinos and power supply used to run four flow systems simultaneously. Picture taken from the Burkart Laboratory, UCSD. .

A second cost-effective solution to flow chemistry was created by engineer David Florian and published to his website Dr. D-Flo. This system is similarly open access, and can be created with a 3D printer and parts ordered from McMaster-Carr and Amazon for a total cost of \$200. Also operated with a stepper motor and Arduino, the main external difference between this system and the Croatt Research Group's is the use of an aluminum rail as opposed to a fully 3D printed chassis. Figure 5 displays David Florian's syringe pump design as manufactured by the Burkart Laboratory, UCSD.

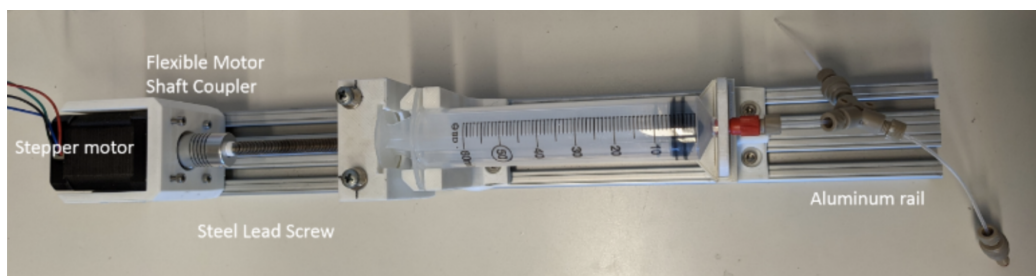


Figure 5. David Florian's syringe pump design.

This design presents the same issues as the Croatt Research Group's in terms of non-intuitive user-input commands, limited wire management solutions, and corrosion of the steel lead screw. Syringes of sizes ranging from 15 to 50 mL can be used with this system. However, changing the size of the syringe requires modifying the 3D printed syringe holders.

A much more expensive syringe pump system that was found during the research process is the Standard Infusion Only PHD Ultra Syringe Pumps. This system uses a mechanical driving mechanism that resembles the Croatt Group's mechanism as it features a lead screw that when rotated by a stepper motor pushes a carriage that pushes the plunger of a syringe. This system also includes two low-friction guiding linear shafts for the carriage and a modular syringe holder design. The main changes we made to the Croatt Research Group's design includes a design change in the syringe holder to facilitate the use of different size syringes. (work in progress) (gonna add specifications next)



Statement of Requirements and Deliverables:

High Priority Objectives:

1. Implement a user-friendly user-interface to serve as a control panel.
2. Design a modular syringe pump that can fit various sizes of syringes (1,3,5,10 mL).
3. Enhance resistance to corrosion of threaded rod.

Second Priority Objectives:

4. Provide an alternative design for refilling the syringe that doesn't rely on expensive check valves.

WOW Design Solution:

5. A system that can detect leaks and shut down the system when they occur.

Deliverables (to be completed):

1. Flow Chemistry System
 - a. 2 complete syringe pumps
 - b. Touchscreen user-interface
2. Documentation
 - a. Manufacturing procedures
 - b. Operation instructions
 - c. Code files
 - d. CAD (Computer Aided Design) files
 - e. BOM

Chapter 2: Description of Final Solution

Functional Requirements

The chemistry flow system must have the following functional requirements:

- Conduct reactions in a continuous flow stream.
- Refill syringes.
- Have an intuitive touchscreen user interface.
- Accurately dispense chemicals for flow rates of 0 to 2 mL.
- Accommodate syringe sizes of 1, 3, 5, and 10 mL.
- Control four syringe pumps simultaneously.

Design Solution

Syringe Pump

The final design solution consists of a total of four major components. The first component is the syringe pump system itself. The system consists of a 3D printed chassis, carriage, and syringe holder, as well as two linear rods, a threaded rod, a linear coupler, and a Nema 17 Stepper motor, as can be seen in Figure xx. The threaded rod in conjunction with a nut embedded in the carriage translates the rotational motion of the stepper motor into linear motion of the carriage which is guided by linear rods. As the stepper motor rotates, so does the threaded rod and the carriage is either advanced forwards or backwards depending on whether a dispensing or refilling input is specified by the user. The plunger of the syringe is mated in a slot on the carriage and so as the carriage moves so does the plunger of the syringe in order to draw in or extrude chemicals from the syringe. The motion of the system can be seen in Figure xx.

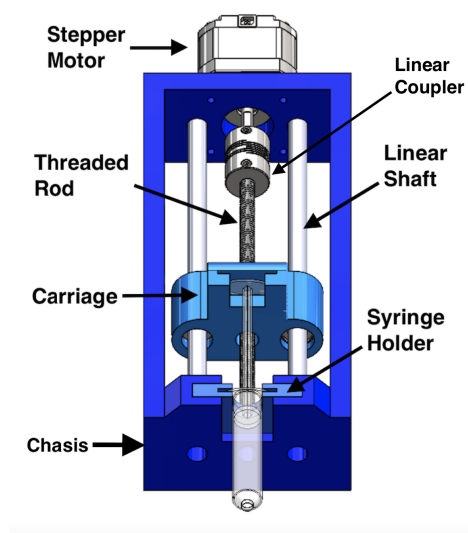


Figure xx. Main Syringe Pump Components.

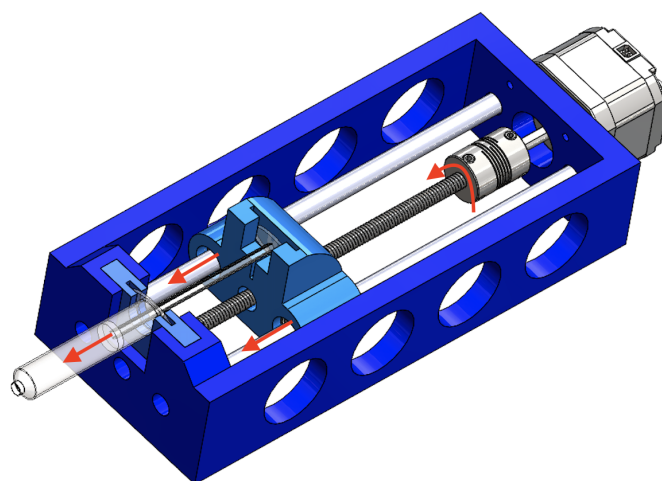


Figure xx. Indication of Motion.

Refill Design

The second major component of the flow system is the servo motor - stopcock refill mechanism. The parts for this mechanism include a servo motor, 3 way stopcock, 5 volt power supply unit, and 3D printed parts to both mount the servo - stopcock mechanism to the system and to mate the servo motor with the stopcock latch. The stopcock valve is able to control the direction of the flow between the refilling and dispensing stages depending on the position of the stopcock latch. For refilling the syringe the stopcock latch is oriented such that the flow channel from the chemical reservoir is open, but the flow channel into the main tubing where reactions take place is closed. When the user sets the status of the syringe to dispensing mode the latch of the stopcock is flipped by the servo motor to allow chemicals to flow into the main tubing, but restrict flow to the chemical reservoir.

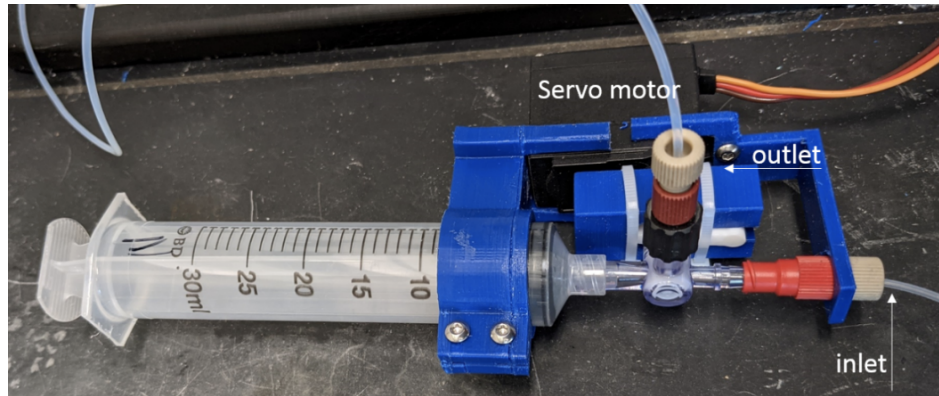


Figure xx. Servo motor-Syringe-Stopcock Connection. [Burkart Laboratory].

User Interface

The third major component is the user interface that is to control the system. The user interface includes both the hardware and the graphical user interface (GUI) design. The user interface hardware selected for our final design is the Nextion 7" Basic Series touchscreen display because it includes both the necessary hardware and software for graphical user interface design. The key functionality of the graphical user interface is for the user to interact with a menu where parameters such as syringe size, flow rate and mode can be set with buttons and then be sent as commands to the syringe pump system. The user interface must also be able to display the current position of the syringe to allow one to monitor the process in real time. The control of the system is handled mainly by the Arduino and motor drivers, which make up the fourth major element of the design.

Electronics and Code

The fourth major element of the design is the electronics and code. The electronics feature an Arduino Mega 2560 and one motor driver for every stepper motor in the system. The code to control the system was written using the Arduino software. The only external library used in the code is the AccelStepper library. We chose to use this Arduino library to control the stepper motors because it allows for multiple stepper motors to be controlled simultaneously. Serial communication is used for communication between the Arduino and Nextion touchscreen. A schematic of the electronics wiring for the entire system can be seen in Figure XX.

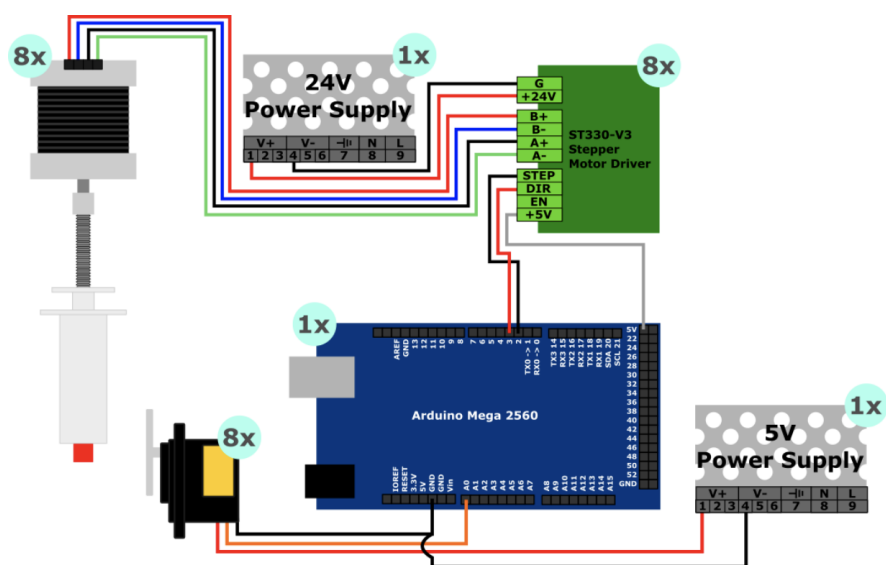


Figure xx. Electronics Schematic. [Burkart Laboratory].

Each of these four components come together to make up the flow chemistry system. The user interface sends commands to the Arduino, which in turn controls the motors and functionality of the syringe pump. As the syringe pump is operating, the refill apparatus ensures that the flow of chemicals is in a singular direction. Figure XX. displays a simple schematic of how each component operates within the flow system as a whole.

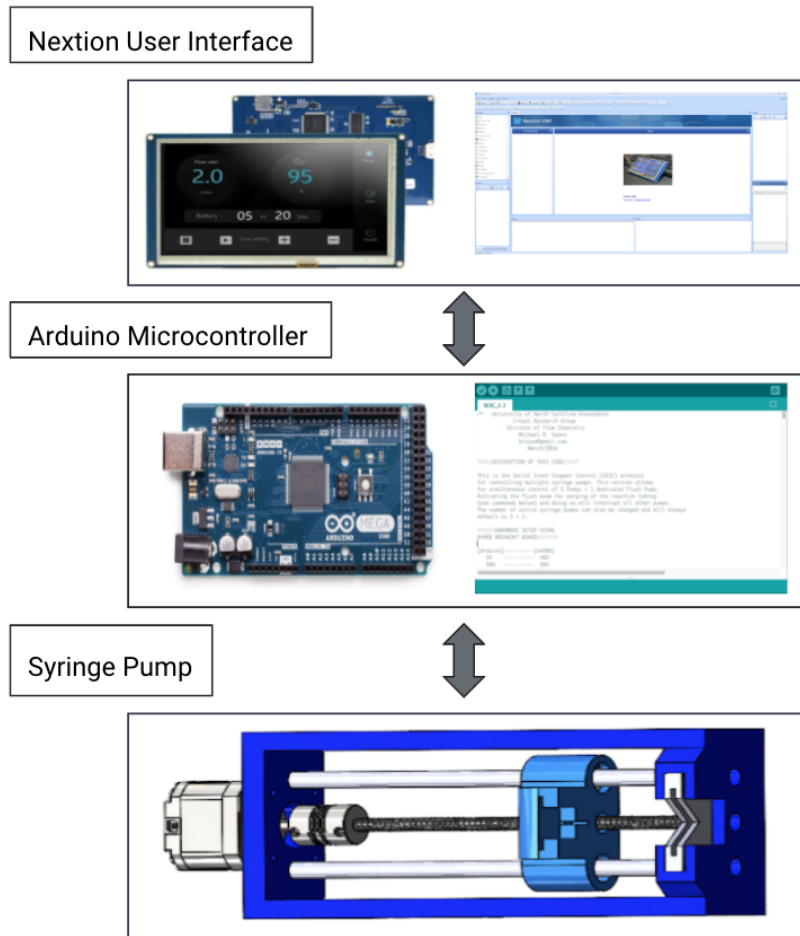


Figure xx. Schematic of System Connections.

Performance Results

(TBD)

Chapter 3 : Design of Key Components

Major components:

- Graphical User Interface (GUI)
- Microcontroller
- Modular Syringe Holder
- Electronics Containment Box
- Lead Screw Actuator

Graphical User Interface (GUI)

An important aspect of this system is having a suitable user interface that is easy to understand and use. The system is to be used by students and others looking to get into chemistry, and this audience might not have much experience handling electronics and programming. As such, it is essential to have an interface that can be operated by anyone.

Initially, there were a variety of different options that could be used for this interface. The existing design from the Croatt Research group utilized a bluetooth app as a way to control the syringe pump. While this is a valid solution, it requires an Android phone and users may be resistant to the idea of having an app for work or school installed on their personal devices. One could buy a low-cost Android phone specifically for the purpose of this system, but even the lowest prices range around \$100. In addition, the app that the Croatt Research group developed was removed from the app store, so any app would have to be fabricated from scratch.

Another possibility was having an LCD screen with a physical control panel of knobs and sliders that can be used to adjust the settings of the syringe pump system. This is a simple solution and would work for a very basic use of the system. However, if someone wanted to build this system with a control panel like this, they would need basic knowledge of how electrical components work and how to integrate them into the system. While it is feasible and instructions can be provided, a touchscreen interface is generally easier to work with. The touchscreen interface greatly reduces the total amount of wiring needed in the system because it only requires a single cable connection, versus the multitude of connections which would be needed to implement a control panel. In addition, LCD displays generally come in smaller sizes, so to display all the wanted data, multiple screens or one large screen would be necessary. However, with a larger LCD screen, it is not much of a leap to simply go with a touchscreen LCD display. The price point is quite similar and any additional settings and options can be handily developed for the touchscreen device. With the non-touchscreen display and the control panel, more physical buttons and such would need to be bought and integrated into the control

panel. In the end, under the guidance of this project's sponsor, a touchscreen device was chosen to be the user interface as it is very adaptable and is easy to use.

Functional Requirements

The user interface must be able to send commands to the microcontroller in order to control the servo and stepper motors. It must also be able to receive data regarding the current position of the stepper motors from the microcontroller. Also, as the setting for this system will be in a chemistry lab, it would be important that the touchscreen is suitable for this environment. The touchscreen will have to be a resistive type as those types of touchscreens can be operated when wearing a glove or with a stylus. Capacitive touchscreens are the other common type of screen, but these touchscreens rely on the conductive properties of the human body. So, this would require that users use their bare fingertips when using the touchscreen, which can be quite dangerous in a lab full of chemicals. Furthermore, since chemicals could accidentally come in contact with the screen, a stylus would be used as well as a suitable screen protector to prevent damage.

Comparison of Designs Considered

	Nextion 7" Basic Display	Adafruit Touchscreen	Touchscreen with Arduino shield
Dimensions	7" x 3.4"	4.7" x 3"	7" x 4"
Screen Type	Resistive	Resistive	Resistive
GUI Design Software	Nextion Editor	None, code from Arduino	None, code from Arduino
Cost	\$90	\$40	\$70

Table XX. Comparison of GUI Design Considerations

Final Choice

The Nextion Basic HMI Display touchscreen was selected as the user interface in the final design. The Nextion touch screen has a lower learning curve when compared to other user interface software design due to its free Nextion Editor Software which features drag-and-drop

components. Of course, the touchscreen is resistive so that it will work even when users are wearing gloves or operating the touchscreen with a stylus.

The Nextion touchscreen is a little more expensive than all the other options considered, but its software allows developers to easily design a GUI by dragging in components such as buttons and sliders. Touch events can be coded in the software with simple commands and the Nextion can output data via Serial communication, perfect for communicating with the Arduino. This saves a lot of time for developing the GUI as elements do not need to be coded in by hand, and it is easier to work on the display if you can see what is going on as you edit the screen.



Figure xx. Nextion Basic Series 7” touchscreen display

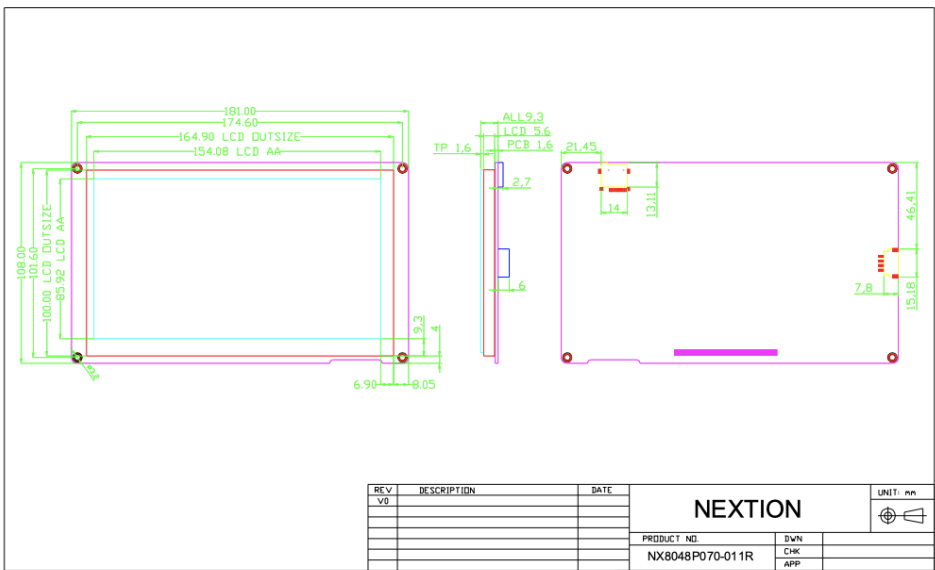


Figure xx. Nextion Basic Series 7” Dimensions.

Software and Programming

The Nextion Editor Software allows buttons and text to be programmed according to one's needs. It can also print information over Serial to a microcontroller. Essentially, this is the method of communication currently being used between the touchscreen and Arduino. Once the data is done printing over to the Arduino, it is just a simple matter of processing the string and changing the parameters of the system accordingly. This software provides a significant advantage as opposed to designing the user interface from scratch, and was therefore a key factor in the decision of the user interface selection.

Microcontroller

The Arduino Mega 2560 was chosen as the microcontroller to be used in the design. This particular Arduino meets all of the functional requirements listed below, and has a number of other positive attributes.

Arduino is an open-source hardware and software company. Arduino products are cost effective and may be interfaced to various other circuits and breadboards. Arduino is one of the most commonly used brands of microcontroller and can be purchased from a number of suppliers for low prices.

After comparing various Arduino and Raspberry Pi microcontrollers, the Arduino Mega 2560 was selected as it is easily accessible and inexpensive.

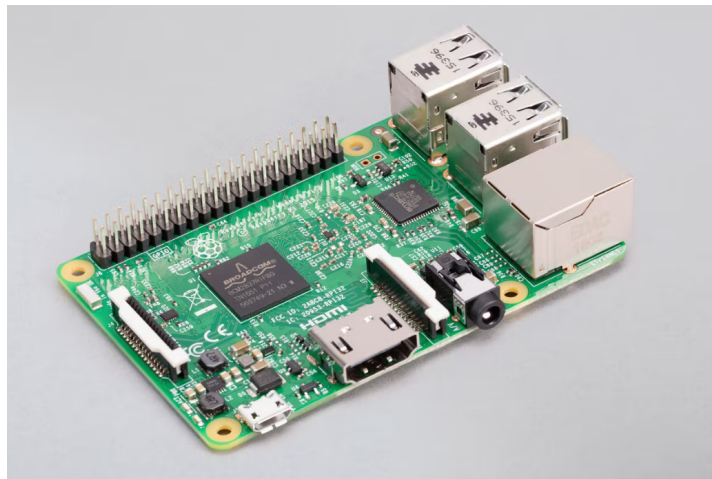


Figure xx. Image of Raspberry pi 3 [From Raspberry Pi store]

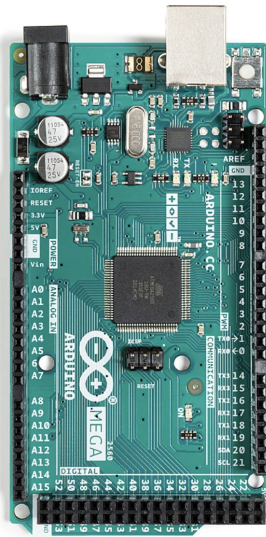


Figure xx. Image of Arduino Mega 2560
[From Arduino store]

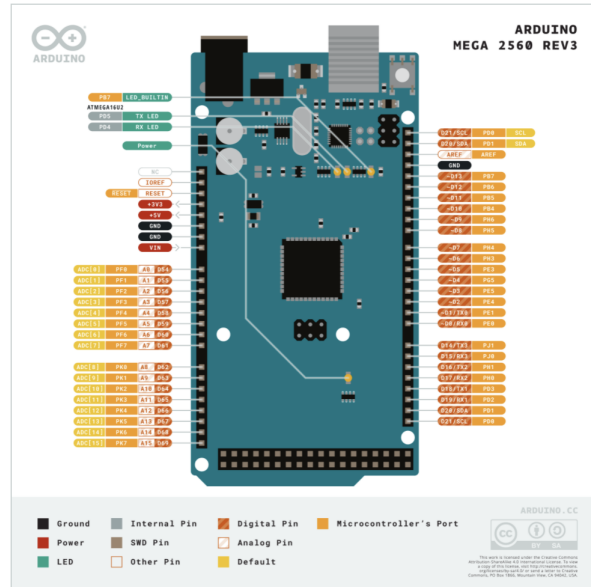


Figure xx. Pinout Diagram of Arduino Mega 2560
[From Arduino store]

Functional Requirements

The microcontroller must be able to control four stepper motors and four servo motors. Therefore, it must have eight digital pins (two for each motor driver) and four analog pins (one per servo motor). In addition, the microcontroller should have pins reserved for Serial communication (a TX pin and RX pin). Generally, most Arduinos have these pins on digital pins 0 and 1, so these should be reserved only for Serial communication (not counted with the other eight pins required for the stepper motors). The microcontroller must also have an available 5V pin and the ability to connect to a power supply or wall outlet. This enables the user to use the system without an external power supply which would reduce the total cost of the system.

The microcontroller must also be able to interface with the GUI. It must be able to receive commands from the GUI over Serial and receive position data from the motor (from the AccelStepper Library).

Comparison of Designs Considered

	Arduino Mega 2560	Arduino Uno Rev3	Raspberry Pi 3 Model B
Operating Voltage	5V	5V	5v

Input Voltage (recommended)	7-12V	7-12V	4.75-5.25V
Input Voltage (limit)	6-20V	6-20V	4.75-5.25V
Digital I/O pins	54	14	26
Analog Input pins	16	6	14

Table XX. Comparison of Microcontroller Design Considerations

Justification of Final Design Choice

The Arduino Mega 2560 was ultimately selected to be used in the final design. The choice of microcontroller was first narrowed down to an Arduino due to their immediate compatibility with the code provided by both the Croatt Research Group as well as the Burkart Laboratory. The Arduino Mega 2560 was selected due to its greater number of digital I/O pins which will allow for additional syringe pumps to be added to the system if desired. However, any Arduino model with a sufficient amount of pins will suffice for this system.

Electronics Containment Box

The electronics containment box is intended to house all of the electrical components excluding the power supplies. It also serves as a mount for the user interface.

Functional Requirements

The electronics containment box must provide an enclosure for the electronics and have multiple points of exit for the wires to extrude from. It is important that there is sufficient room for the wires to protrude from each of the components so that the bend radius of each wire is not exceeded. Easy access to the wires and electrical components should be maintained at all times, therefore there should be no permanent sealing of the box.

The electronics containment box must:

- Fits four motor drivers, one Arduino Mega 2560, one breadboard.
- Mount the user interface.
- Provide easy access to all connections and electrical components.
- Provide necessary cooling to all components.

The containment had to be designed to be properly ventilated to reduce heating of the motor drives and the controllers. The power supply including the additional 5v supply for the servo motor remain outside the containment in order to reduce complications with cooling.

Comparison of Designs Considered

The first design featured a single solid structure with openings to place the components and the touch screen. However this design faced numerous complications

- 3 D printing the singular solid structure was not possible as the dimensions exceeded the limit of the 3D printer.
- Tight fitting of all the components resulted in wires disconnecting and causing issues with the functioning of the system.
- Once assembled, the interior electronics are not easily accessible in order to make corrections or changes.

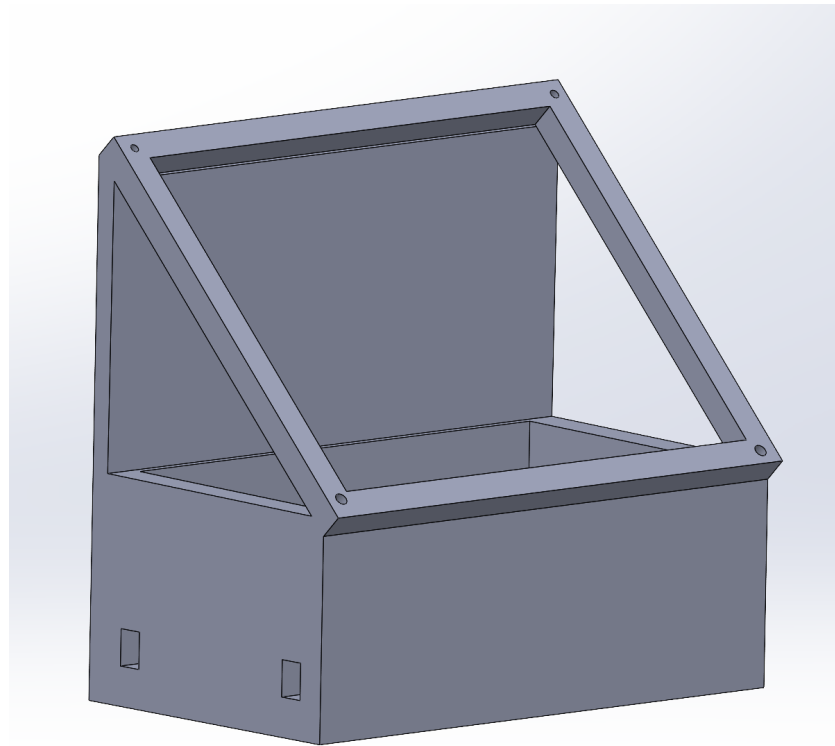


Figure xx. Electronics Containment Preliminary Design

The second design was then modeled where the entire enclosure would be made out of two parts to fix most of the issues. The top lid and the bottom container would fit using snaps. However, the design considered was not made with respect to the limitations of the 3D printer bed. Therefore, it had to be scaled down and the layout of the components inside the box had to

be rethought in order to reduce the footprint of the box. Also, 3D printing snaps were not efficient as they were not accurate after the print.

The third design fixed these constraints. The two parts were scaled down in order to be easily printed on a 3D printer. The lid was fitted using a rail mechanism. This made it easier to access and assemble the electronics. There was a slot and a rest made on the lid for the placement of the stylus.

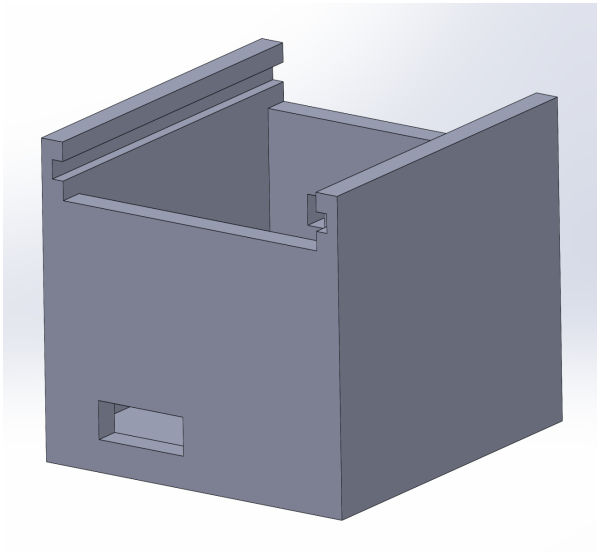


Figure xx. Electronics Containment Box
(resized and edited to support the new
orientation)

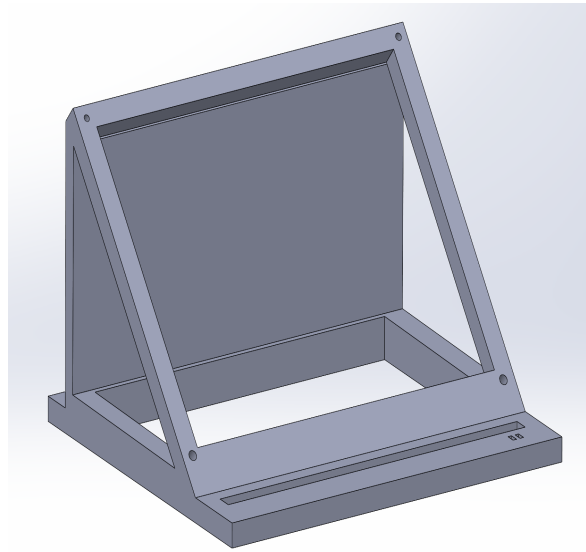


Figure xx. Electronics Containment Box Lid

Lid Design

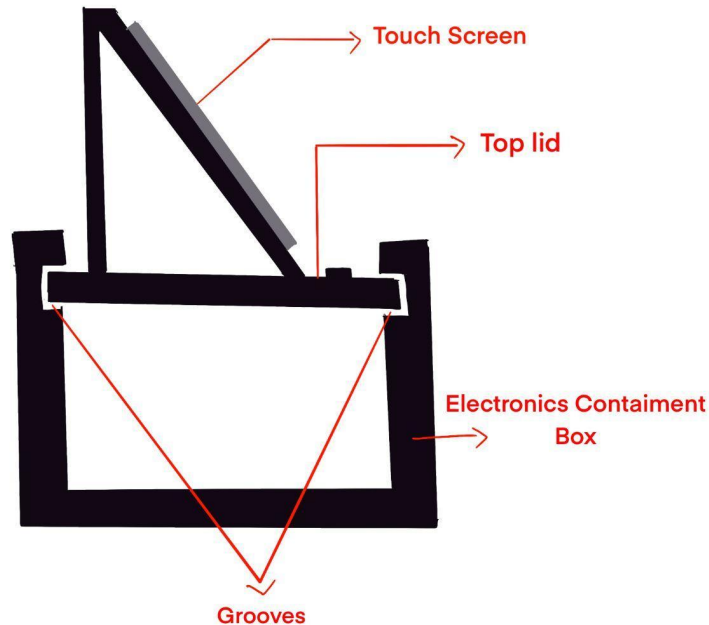


Figure xx. Lid fitment with the electronics containment

User Interface Mounting Design

(insert CAD of angled lid with user interface included – maybe an exploded view of how the screws will mount it)

Modular Syringe Holder

The modular syringe holder is one of the high priority objectives in the project proposal. The syringe holder is intended to be capable of holding syringes of 1, 3, 5 and 10 mL capacity without any alterations being made to the system.

Functional Requirements

The syringe holder must be capable of securely holding syringes of 1,3,5 and 10 mL capacity.

Comparison of Designs Considered

The first design under consideration utilized a screw with a hex nut embedded into a slot that is inside the ledge of the chassis in order to hold the syringe securely in place as can be seen in figure xx. The barrel of the syringe rests on the triangular shaped chassis design which provides the advantage of being able to fit any size syringe. The flange of the syringe (refer to figure xx for syringe anatomy) is captured within a thin slot so that the syringe is fixed in place when force from the carriage is applied to it. A screw with a knob on one end and a plastic cap on the other would be used to tighten down on the barrel of the syringe to provide extra resistance to motion. In order to avoid the issue of not being able to tap 3D printed material, this design includes a nut inserted into a cavity in the 3D print so that the screw has threads to properly rotate within. Another solution to this issue is a heat set insert, however this was avoided due to extra manufacturing steps that it would create.

Some advantages of this system include providing resistance to vertical motion which provides a safety mechanism for the system. Another advantage of this design is that minimal extra hardware would be required as the stock threaded rod would provide the screw piece needed and nuts would have been purchased already. Therefore, the only required components would be the knob and the plastic cap. The knob can even be 3D printed which leaves only the cap to be purchased. One more advantage for this design is that it can be easily assembled as all that is required is for the hex nut to be inserted into a pocket which is identical to the pocket found in the carriage. The other assembly required would be that of super gluing the knob to one end of the threaded rod and slipping the plastic cap to the other end.

While this design satisfies the necessary requirements of the syringe holder, there are a couple of disadvantages with it. There is potential for an inexperienced user to overtighten the syringe which may lead to inaccurate volume predictions as well as a worst-case scenario of the plastic syringe permanently deforming if too much pressure is applied. Additionally, the screw and nut system does not provide a locking mechanism to secure the screws' position. Therefore the screw may loosen and no longer provide sufficient force to properly hold the syringe in place.

For the added safety of this syringe holder design one might be inclined to spend extra if they intend to use a larger stepper motor which will be able to provide larger translational forces.

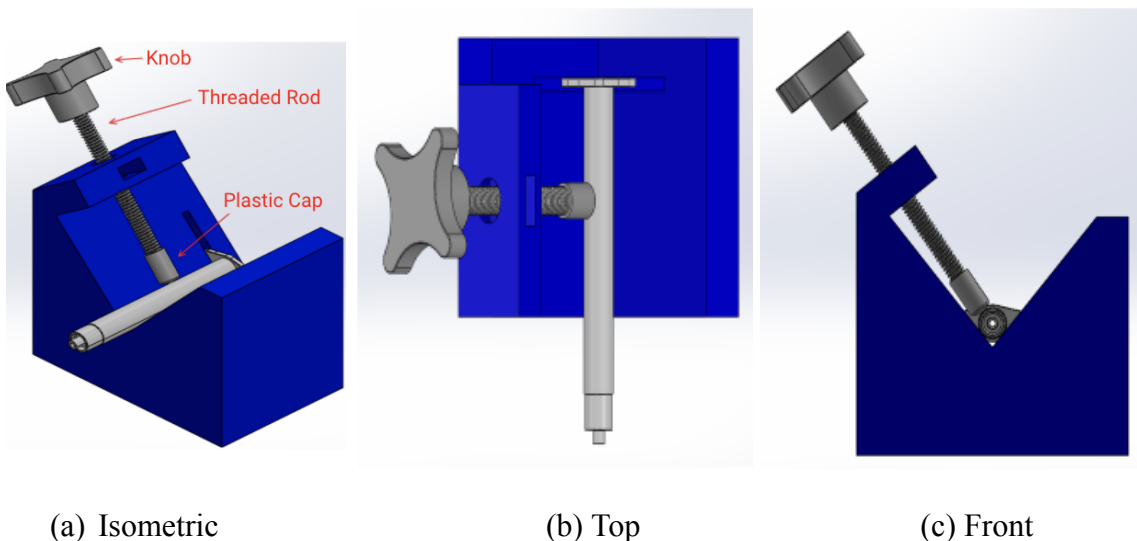


Figure xx. Set Screw Modular Syringe Holder

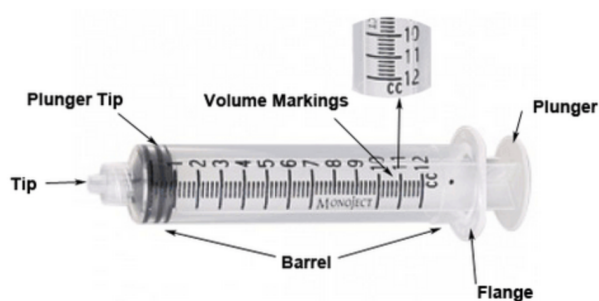


Figure XX. Anatomy of a Syringe. [Vitality Medical].

The second design considered was the syringe holder designed by the Mass Spectrometry Research Group with the Analytical Chemistry Division in the Chemistry Department of Moscow State University as seen in Figure xx¹.

¹ Samokhin, Andrey. "Open-Source Syringe Pump." *Группа Масс-Спектрометрии*, www.mass-spec.ru/projects/diy/syringe_pump/eng/.

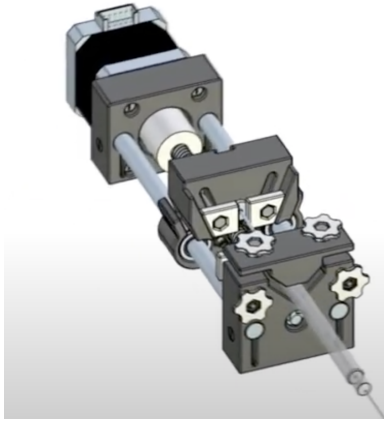


Figure xx. Full syringe pump model. [Mass Spectrometry Research Group, Open Source Syringe Pump].

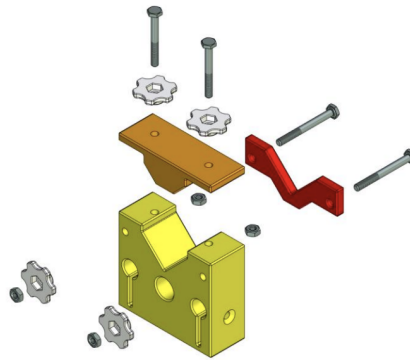


Figure xx. Assembly instructions for syringe holder. [Mass Spectrometry Research Group, Open Source Syringe Pump].

While this design has its merits and fulfills the functional requirements of the syringe holder, it also has a number of the same disadvantages as the previous design. The need to tighten screws to secure the syringe allows for the possibility of overtightening. This design also requires additional hardware and assembly as seen in Figure xx. Therefore, a third design was developed.

The third design considered is pictured in figure xx. This design has a number of advantages over the previous two designs. No additional hardware is needed for this design. This decreases cost, complexity, and potential manufacturing errors. Another advantage of this design is that it can be inserted into the original chassis design so that no extra filament is needed to create the design.

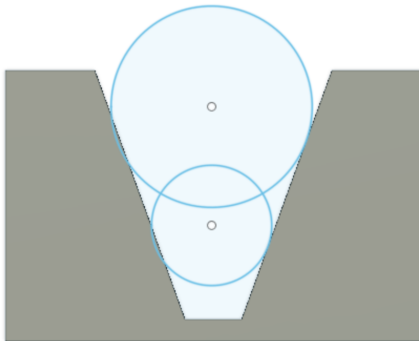


Figure xx. Syringe holder model with circles to indicate fit of various syringe sizes.



Figure xx. Syringe holder with 1mL and 5mL syringes.

One disadvantage of this design is that it provides minimal clamping support to keep the syringe in place which may be a safety concern. The clamping support provided depends on the tolerance between the flange of the syringe and the slot it is inserted in. This tolerance will vary depending on the specific syringe in use as different manufactures use different geometry and thicknesses of the flange. It is possible to modify the design of the syringe holder so that the specific syringe in use will fit within the slot with a press fit rather than a clearance fit and therefore provide sufficient clamping. However, this will require some modification to the CAD files, which may not be in some user's area of expertise. Therefore, the syringe holder in this design allows for some clearance so that multiple types of syringe will fit in the system.

Despite these minor disadvantages, this design was selected as the final syringe holder design due to its fulfilment of the functional requirements of the syringe holder and the overarching project objectives of minimal assembly and cost.

A future design consideration is to embed the syringe holder in the chassis to combine them into a single 3D printed component. Therefore, additional 3D printing and assembly steps would be eliminated. This would also benefit with respect to alignment and accuracy because there would be no potential for the syringe holder to be inserted off center or to not be completely seated in the chassis.

It may also be noted that minor post-processing of the syringe holder was required to remove the remaining support materials from the interior slot for the flange of the syringe. This

was done using tools on hand such as pliers and a small screwdriver to scrape out remaining unwanted filament. Tweezers may also be useful for this task.

Modular Carriage Design

The selected syringe holder design allows for syringes to sit at different heights within the holder. In order to accommodate for the variance in height of each different syringe size, the carriage must also allow for syringe plunger to sit at different heights so that the syringe remains horizontal. The Croat Group's design included a single rectangular slot which didn't allow for the plungers to sit low enough to match the height that the smaller diameter syringes sit in the syringe holder. Therefore, a simple modification to the carriage was made by adding a triangular cutout. Like with the syringe holder, this triangular geometry allows for the syringe to sit at the proper height.

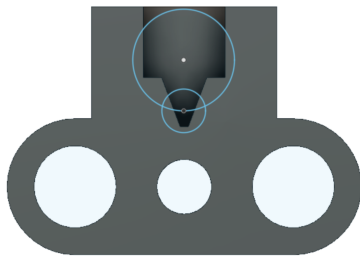


Figure xx. Carriage model with circles to indicate fit of various syringe sizes.

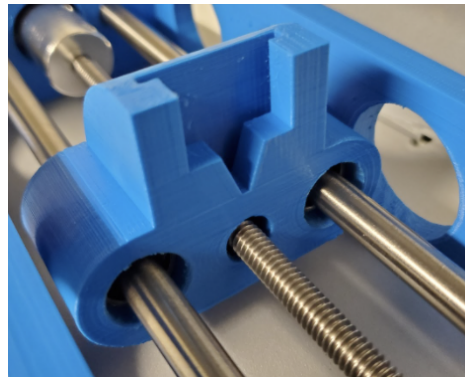


Figure xx. 3D printed Carriage.

A similar issue with the tolerance of the slot as was observed with the syringe holder appeared with the carriage design. The varied thickness of different syringe plungers leads to a clearance fit between some syringe plungers and the slot it sits within. This gap would cause discrepancies in the measurements due to the motor moving through the distance of the gap before the plunger is engaged and liquid is expelled or retracted. This issue may be solved as mentioned earlier - by modifying the carriage design in order to provide a press fit for the specific syringe in use.

After 3D printing the third design of the modular syringe holder and the modified carriage, it was verified that this combination is a viable design. The syringe holder fits syringe sizes of 1,3,5, and 10 mL as outlined in the functional requirements and the syringe is held horizontal due to the modifications made in the carriage.

Lead Screw Actuator (work in progress)

Single handedly the most important component of the syringe pump system which will determine the performance of it, the lead screw actuator is the mechanism which provides the force to move the syringe plunger and it refers to the system that includes the Nema-17 stepper motor, threaded rod and hex nut.

Functional Requirements

The functional requirements of the lead screw actuator is that it must allow for the accurate linear positioning of the carriage which in turn allows for the control of the flow rate of the syringe pump system based on the velocity of the stepper motor as well as other parameters.

Comparison of Designs Considered

1. **Threaded rod (screw) with nut**
2. **Ball screw**
3. **Pre-coupled Lead Screw w/ stepper motor**

Designs Considered	Pros	Cons
Threaded Rod with Nut	• Already bought • Easily accessible • Low cost • Accurate (...) • Corrosion resistant	• Can be more accurate • Low screw efficiency (...)
Ball Screw with Nut	• More accurate (...) •	• More expensive () • Not as easily accessible
Pre-Coupled Lead Screw with Stepper Motor	• No coupling required	• Expensive (\$67.64) • Higher step resolution (0.024383 mm/step) • Lower maximum

		linear force (250 N) • Not as easily accessible
--	--	---

Justification of Final Design Choice

From the lead screw analysis it was found that the maximum theoretical linear force that is provided by the motor is This result is significant because it provides a conservative maximum baseline for the output linear force of the motor. To see the magnitude of forces that would be present during the operation of the syringe pump system, an analysis to estimate the theoretical pushing forces needed to get a specific flow rate from a syringe was done. The results received for a 2 mL/min flow rate were that forces between And would need to be provided for syringe sizes ranging from 1 mL to 10 mL. These results therefore show us that the motor we have chosen provides more than enough linear force to operate the syringe pump system effectively.

Chapter 4 : Prototype Performance

Theoretical Predictions

Theoretical predictions regarding the performance of the flow chemistry system were determined through experimentation are as follows:

- The maximum syringe size that the motor will be capable of pushing is (##) determined by the analysis on page xxx.
- The maximum flow rates that the syringe pump at which the syringe pump will be able to reliably operate for a variety of syringe sizes are listed in the table below:

Syringe Size	Dispense Resolution [$\mu\text{L}/\text{step}$]	Max Flow Rate [mL/sec]	Max Flow Rate [mL/min]
1 mL	0.0922	0.1844	11.064
3 mL	0.3862	0.772	46.32
5 mL	0.7062	1.412	84.72
10 mL	1.063	2.126	127.56

Table xx: Maximum Flow Rates for given Syringe Sizes

- The flow rates of each syringe pump will be within $\pm(\##)$ of the programmed flow rate. (Maybe separate accuracy by syringe size/ flow rate if they're different and add another table).

Test Conditions

Maximum Syringe Size

In order to verify the maximum syringe size that the syringe pusher is capable of pushing reliably, syringes of increasing size were inserted into the syringe pump and the stepper motor was initiated at a specific flow rate. Reliable operation of the stepper motor was determined by measuring the output flow rate. If the stepper motor reaches a point where it is not capable of providing sufficient torque output to overcome the force needed to advance the carriage and push the plunger of the syringe, it will skip steps

in its rotation. When this occurs, the flowrate will be lower than expected due to the decreased aggregate rotation of the motor.

First, a baseline flow rate was recorded with a 1mL syringe. This baseline was recorded with a syringe that the motor is assuredly capable of pushing because every syringe pump will have slight inconsistencies which lead to a flow rate slightly different than the programmed flow rate. Therefore, by comparing the measured flow rate with increasing syringe sizes to the baseline flow rate, it was evident when the flow rate no longer matched the baseline flow rate, indicating that the stepper motor did not have sufficient torque to push the syringe.

After the baseline flow rate was recorded, syringes of increasing size were placed in the system and the flow rate was recorded and compared with the baseline.

Maximum Flow Rate

The maximum flow rate that the syringe pump can operate at is determined by the maximum speed of the stepper motor. In order to verify the accuracy of the analysis performed, increasing flow rates were programmed and the measured flow rate was recorded. The maximum flow rate was determined when the increasing speed no longer increased the measured flow rate.

Accuracy of Flow Rate

The accuracy of the flow rate was determined by running multiple experiments with various syringe sizes and recording the measured flow rate. These experiments were performed with the two flow systems on hand which were both manufactured with the same 3D printer. Therefore, these accuracy ranges unfortunately do not include the accuracy of systems manufactured with different printers. However, these measurements may provide a baseline to which flow rate deviations in other syringe pumps can be compared.

Results

(TBD)

Comparison of Results to Initial Performance Requirements

(TBD)

Chapter 5 : Design Recommendations and Conclusions

Design Recommendations for the Future

Incorporate Real-time Flow Rate Sensing Capability

Due to the DIY nature of the project it is impossible to attain uniform results. Variations in the model of 3D printer used, 3D printing settings and conditions, tolerances of the hardware, as well as variations in the brand and model of syringes used all contribute to discrepancies between any two given systems. As such, the flow rate dispensed by each syringe pump may differ slightly from the programmed flow rate as well as from the other syringe pumps being used with the system. This is an issue due to the stoichiometric ratios not being maintained. Without proper stoichiometric ratios, reactions will not take place as intended and losses of supplies, time, and money may occur.

In order to avoid these discrepancies each syringe pump must be calibrated before usage. As the system currently stands this calibration entails measuring the volume extruded from the syringe pump for a recorded amount of time, then manually calculating the flow rate from these results. Once the actual flow rate is known for a range of programmed flow rates, values can be entered to create equal flow between the syringe pumps to maintain proper stoichiometry.

This calibration process could be streamlined by implementing real-time flow rate sensing capabilities. By adding a flow-rate sensor to the output valve from each syringe pump

and displaying the flow rates to the user interface, users would be able to see the flow rates in real-time. This would significantly reduce the effort required in the calibration process and make accurate, real-time adjustment of the flow rates possible.

Leak Detection System

In some cases it may be desirable to run reactions over extended periods of time. In these cases it would be convenient to leave the system unattended as the reaction is carried out. However, extreme care must be taken to ensure that no chemical spillages occur when the system is unattended.

This device is currently not suitable for unsupervised use due to its lack of automated monitoring and emergency shut off controls. A chemist is needed to supervise the system in the case a blockage or leak in the system occurs. If such an issue occurs, the chemist supervising the experiment must detect the issue and manually shut off the system to avoid chemical spillage.

Ensuing implementation of real-time flow rate sensing as previously mentioned, autonomous detection of leaks or blockages in the system would be possible. If the flow rate is much higher than expected a leak may be present in the system. If the flow rate is lower than the expected, this would be an indication that there is a blockage obstructing the flow. Therefore, the ability to detect flow rates would allow for the implementation of an automatic shut off command which shuts off the system if the measured flow rate indicates that a leak or blockage has occurred. The addition of an automatic shut off command would enhance the overall safety of the system and allow for a flow system that is safe to leave unattended for extended periods of time.

Safety Considerations

Safety considerations for this project relate to the use of chemicals within the flow system, electrical wiring, and 3D printing protocols.

When dealing with chemicals proper laboratory protocols should be followed at all times. Experiments should be conducted with the flow pump system within a closed fume hood.

If a leak or blockage is detected the system should be shut off immediately. As the design currently stands, the flow system should never be left unattended.

With respect to the electrical components in the system, it is important that the wiring diagrams be followed so that no short circuits are created. A short circuit may produce sparks, smoke, or fire. This may result in personal injury, as well as permanent damage to the electrical components in the system.

Operation of the 3D printer is another area of potential risk. To mitigate this risk, it is important to follow the operating instructions of the specific 3D printer being used. 3D printers are generally safe machines, although care must be taken to avoid touching the heated components of the printer. The nozzle of the printer is generally heated to 210 - 250°C and the bed to 60 - 110°C. If contact with the skin occurs a burn may result. Additionally, when removing supports from the finished 3D printed components, care must be taken to not scratch oneself on the rough support material.

Engineering Standards

Restriction of Hazardous Substances (RoHS)

The Restriction of Hazardous Substances (RoHS) Directive (2002/95/EC) regulates the use of hazardous substances in electronic devices². The RoHS Directive was adopted by the European Union in 2003. California adopted the directive in 2003 as well but under a limited scope. The hazardous substances limited by California Senate Bills 20 and 50 include four of the ten substances limited by the RoHS Directive, those being lead, mercury, cadmium, and hexavalent chromium. Another directive which sets standards for electronic equipment is the Electromagnetic Directive (EMC) (2014/30/EU). A device is EMC compatible if it is able to function acceptably in its electromagnetic environment. This includes limiting the unintentional generation, propagation and reception of electromagnetic energy, all of which may cause unwanted effects such as electromagnetic interference (EMI) or physical damage in operational

² *RoHS Directive*. Environment. (n.d.). Retrieved January 29, 2022, from https://ec.europa.eu/environment/topics/waste-and-recycling/rohs-directive_en

equipment³. The electronics in this design were selected to be compliant with the RoHS and EMC directives. Specifically, the Nextion 7” Basic Series Display and Arduino Mega 2560 are both RoHS and EMC compliant.

ASME Y14.5 Dimensioning and Tolerancing

The ASME Y14.5 Dimensioning and Tolerancing standard is applicable to this project due to the use of CAD files in order to design the 3D printed components. This standard creates a common technical drawing language for standardized drawing practices and has been revised over the years to be compatible with electronic systems, such as Computer Aided Design (CAD). This standard was therefore applied when creating the CAD files for the 3D printed components of the system.

ANSI Internal and External Thread Classes

ANSI Internal and External Thread Classes is a widely adopted standard for thread screw classes which specifies the degree of tightness between threaded components⁴. Thread screw classes specified in the ANSI Thread Classes represent manufacturing tolerances that specify minimum and maximum pitch diameters for both internal and external threads. The stainless steel threaded rod used as the linear actuator in the syringe pump system is sized with ANSI class 2A external threads. This class is intended to maximize the strength of the threads, and is therefore an advisable choice for this design since the threaded rod and nut are used to translate rotational force to linear force acting on the syringe. The tolerance allowed for a class 2A lead screw is a minimum pitch diameter of 0.2127 inches and a maximum pitch diameter of 0.2164 inches. The threaded rod in the system is paired with a ANSI class 2B steel hex nut which

³ EMC Directive 2014/30/EU. cemarking.net. (2022, January 3). Retrieved January 29, 2022, from <https://cemarking.net/eu-ce-marking-directives/emc-directive/>

⁴ Edge, Engineers. “ANSI Internal and External Thread Classes: Engineers Edge.” *Engineers Edge - Engineering, Design and Manufacturing Solutions*, www.engineersedge.com/thread_strength/thread_classes.htm#:~:text=There%20are%20three%20classes%20of,play%20or%20clearance%20in%20assembly.

has an allowed pitch diameter ranging from a minimum of 0.2175 inches to a maximum diameter of 0.2248 inches.

Chemical Hazards and Toxic Substances

OSHA (Occupational Safety and Health Information) has standards regarding Chemical Hazards and Toxic Substances. Controlling Exposure is a section of these standards which includes controls such as Elimination/Substitution, Engineering Controls, Administrative and Work Practice Controls, as well as Personal Protective Equipment. The Engineering Controls involve implementing physical change to the work environment which reduces or eliminates the hazard on the job. Examples of such controls include changing processes to minimize contact with hazardous chemicals, isolating or enclosing the process, use of wet methods to reduce generation of dust or other particles, general dilution ventilation, and the use of fume hoods⁵. This flow system has been designed to adhere to these standards. Specifically, the automatic refill option was designed to minimize contact with hazardous materials. In the Croatt Research Group's original design, the chemist is required to fill a syringe by hand, install it in the syringe pump, and refill the syringe when necessary. With the automatic refill, the need for contact with and transportation of a syringe full of hazardous materials is eliminated by automating the process once the syringe has already been placed in the syringe pump. Additionally, the design of this flow system was made to control exposure by accommodating the use of fume hoods. Extended wires between the syringe pump and the GUI allow for the syringe pump to be placed in an enclosed fume hood while the GUI and electronics sit on a nearby surface. Therefore, the portion of the system in contact with chemicals and hazardous substances can be enclosed in a fume hood while the electronics remain operable at a safe distance away. These design choices have been made to act in accordance with OSHA's Chemical Hazards and Toxic Substances standards.

Impact on Society

⁵ *Chemical Hazardous and Toxic Substances*. Chemical Hazards and Toxic Substances - Controlling Exposure | Occupational Safety and Health Administration. (n.d.). Retrieved January 29, 2022, from <https://www.osha.gov/chemical-hazards/controlling-exposure>

Green chemistry (or sustainable chemistry) refers to the development of efficient chemical processes that reduce or eliminate the generation of hazardous substances⁶. It takes into consideration the environmental impact of every step in the process of chemical synthesis, from the waste created during the reaction to the lasting effects that the chemicals created will have on the environment. It also concerns safety, aiming to minimize potential hazards to laboratory personnel. As environmental concerns have come to a head over the past half-century, government, academia, and industry alike have begun to look towards green chemistry as a necessary scientific advancement in order to promote a more sustainable civilization⁷.

Flow chemistry has made valuable contributions towards the practice of green chemistry. By allowing for strict control of reaction parameters, the efficiency of reactions is increased, waste is reduced, and safety is enhanced. However, one important consideration when it comes to green chemistry initiatives is the economic impact of the processes being implemented. Governments, industries, and research institutions desire both environmental and economic sustainability. Practices must therefore be cost effective in order to gain acceptance and widespread use. Currently, chemistry flow systems are prohibitively expensive and therefore largely impractical for large-scale implementation. By greatly reducing the price of flow systems, use of these systems will become more commonplace as institutions no longer have to choose between environmental and economic sustainability. This creates opportunity for a larger portion of chemical synthesis to be conducted in a sustainable manner.

This design will have valuable social implications in addition to its environmental ones. Cost-effective, DIY flow systems have already been developed, however these systems are non-intuitive and not user friendly. The user-friendly nature of this flow system will allow for increased prevalence of flow systems in undergraduate laboratories because students will not require significant training and expertise to operate the system. Therefore, a greater number of students will have the opportunity to conduct experiments using this equipment, leading to a

⁶ Environmental Protection Agency. (n.d.). *Basics of Green Chemistry*. EPA. Retrieved January 17, 2022, from <https://www.epa.gov/greenchemistry/basics-green-chemistry#definition>

⁷ Vaccaro, L., Lanari, D., Marrocchi, A., & Strappaveccia, G. (2014). Flow approaches towards Sustainability. *Green Chem.*, 16(8), 3680–3704. <https://doi.org/10.1039/c4gc00410h>

workforce of adept chemists. Furthermore, by removing unnecessary obstacles associated with operating the system, students will be inspired rather than discouraged when using this flow system. This inspiration will encourage students to persevere through difficult courses, and enhance the retention of students from underrepresented groups in STEM fields.

Professional Responsibility

When designing the system, care was taken to account for the safety of the individuals operating the system. Therefore, an automated refill option has been included to minimize the handling of chemicals by allowing users to command the system to refill the syringes using the user interface. Without this option, the syringes must be detached from the system, refilled by hand, and repositioned within the syringe pump. This process may lead to accidental chemical spills and the chance of chemicals coming into contact with the operator's skin.

While the use of this design advances sustainable chemistry initiatives and therefore addresses environmental concerns, the environmental implications of the production of this system must also be taken into consideration. The majority of the design is 3D printed, and is therefore not intended for long term use. Replication of this design will therefore lead to the creation of plastic waste once the system has reached the end of its lifespan. Most common types of 3D printing filament are classified as Type 7, or “Other” by the ASTM International Resin Identifier Codes⁸. Type 7 plastics are not recycled by most curbside municipal recycling programs and consequently often end up in landfills. However, independent plastic recycling and processing companies exist which process plastics not typically handled by municipal recycling programs. It is also possible to melt down old 3D printed components and re-extrude them as usable filament⁹. Additionally, PLA (Polylactic Acid), one of the most commonly used 3D

⁸ *3D Print Recycling*. Iowa State University Computation and Construction Lab. (n.d.). Retrieved January 17, 2022, from <https://ccl.design.iastate.edu/3d-print-recycling/#:~:text=One%20of%20the%20common%20types,typically%20processed%20by%20municipal%20programs>.

⁹ *3D Print Recycling*. Iowa State University Computation and Construction Lab. (n.d.). Retrieved January 17, 2022, from

printing filaments, is a biodegradable material which means that it can be broken down over time. As 3D printing gains popularity, there is discussion regarding the introduction of more comprehensive recycling codes in order to include common 3D printing filament polymers.¹⁰ Therefore, there are options for recycling the 3D printed components created for the purpose of this flow chemistry system.

Lessoned Learned

(TBD)

Conclusions

(TBD)

Acknowledgements

(tbd)

References

(tbd)

<https://ccl.design.iastate.edu/3d-print-recycling/#:~:text=One%20of%20the%20common%20types,typically%20processed%20by%20municipal%20programs>.

¹⁰ Emily J. Hunt, Chenlong Zhang, Nick Anzalone, Joshua M. Pearce, Polymer recycling codes for distributed manufacturing with 3-D printers, Resources, Conservation and Recycling, Volume 97, 2015. Pages 24-30. ISSN 0921-3449. <https://www.sciencedirect.com/science/article/pii/S0921344915000269>.

Appendix

Users/Maintenance/Safety/Operation Manual

(TBD)

Fabrication Instructions

(TBD)

(3D printing the individual parts

- Electronics casing top lid
- Electronics casing box
- System Chassis (integrated with the syringe holder)
- Syringe Carriage)

Drawings/Layouts/Parts Listing

(TBD)

Bill of Materials

Name	Quantity
Stepper Motor	2
Linear Coupler (4 pc)	2
Ball Bearing Bushings (4 pc)	2
8 mm Linear Rods (2 pc)	1
Fully Threaded Rod	1
Stepper Motor Driver	2
Nextion Touchscreen	1
12V 30A Power Supply	1
Tubing	
3D printing filament	
3 Wire power cord	1
Servo Motor (4 pc)	1
5V 5A Power Supply	1
Stylus Pen	1
Cord Protector Wire	1
Jumper Wires	1

Table xx. Bill of Materials (Not Finalized)

Specification Sheets for Parts Purchased

Product information

Product Dimensions	1.6 x 0.78 x 1.69 inches
Item Weight	7.8 ounces
ASIN	B07GRMRH1Q
Item model number	0510U1J2GPSINM53091A89
Manufacturer recommended age	12 years and up
Best Sellers Rank	#37,221 in Toys & Games (See Top 100 in Toys & Games) #15 in RC Servos
Customer Reviews	 442 ratings 4.2 out of 5 stars
Is Discontinued By Manufacturer	No
Mfg Recommended age	12 year and up
Manufacturer	Seamuing

Table XX. Seamuing Micro Servo Motor, MG995 RC Servo, 20kg Metal Gear Servo for RC Robot Arm Helicopter Airplane Remote Control Product Information.

Additional information

Display Size	7.0"
Resolution	800*480
Touch Panel	RTP
MCU	48 MHz
Flash	16 MB
SRAM	3584 Byte
Input Power	DC 5V 500mA
USART Port	XH2.54 4P
Storage Temperature	-30 ~ 85 °C
Working Temperature	-20 ~ 70 °C
Nextion Editor Components	Text, Scrolling Text, Number, Xfloat, Button, Progress Bar, Picture, Crop, Hotspot, TouchCap, Gauge, Waveform, Slider, Timer, Variable, Dual-state Button, Checkbox, Radio, QRcode
Character Encoding	ascii, utf-8, iso-8859-1~15, gb2312, ks_c_5601-1987, big5, windows-874/1255/1256/1257/1258, koi8-r, shift-jis
Anti-aliasing font	Yes
Product Dimensions	https://cdn.nextion.tech/wp-content/uploads/2017/09/7.0_Nextion_Dimension.pdf

Table xx. Nextion 7" Basic Series Touch Display Specifications

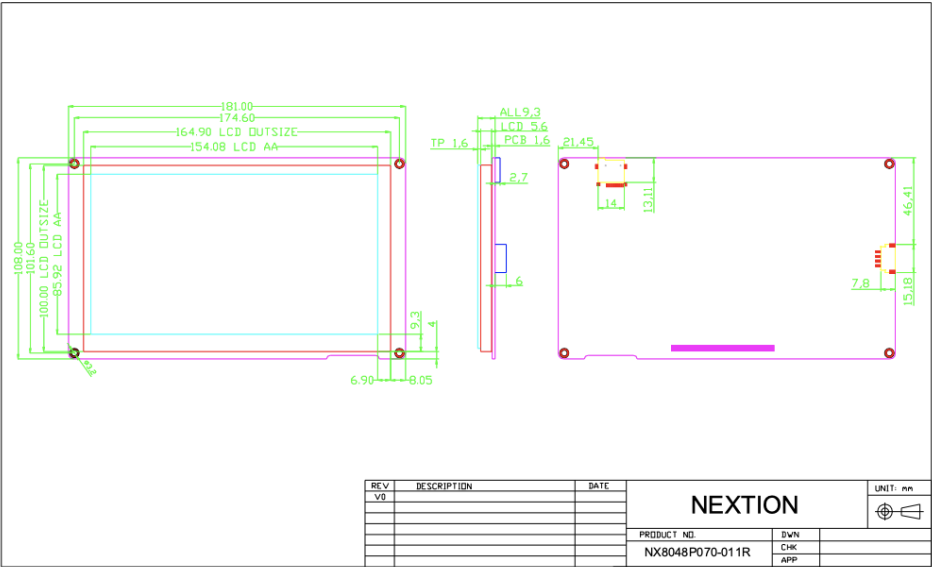


Figure xx. Nextion 7” Basic Series Touch Display Dimensions.

Rev: A

Date:

Nema 17 Stepper Motor

COMMON RATINGS

Step angle :	1.8°	Dielectric strength :	500VAC
Positional accuracy :	±5%	Insulation resistance :	100Mohm(500VDC)
Number of Phase :	2	Ambient Temperature :	-10℃~50℃
Temperature rise :	80℃MAX	Insulation class :	B
Rotor Inertia :	54gcm ²	Weight :	0.3Kg

SPECIFICATIONS

Holding Torque (2 phases on) N.m	Rated Current/Phase (Amps DC)	Phase Resistance (ohms) ±10%	Rated Voltage/Phase (V DC)	Phase Inductance (mH)±20%(1KHz) Typical
0.45	2.0	1.1	2.2	2.6

DIMENSIONS unit=mm

Technical drawing of a Nema 17 Stepper Motor showing side and front views with dimensions.

Side View Dimensions:

- Top flange width: 23±0.5
- Motor body length: 40Max
- Bottom flange width: 2.0
- Bottom flange thickness: 4.5±0.1
- Bottom flange outer diameter: Ø22.0±0.05

Front View Dimensions:

- Outer diameter: 42.0MAX
- Inner diameter: 31.0±0.1
- Mounting hole diameter: Ø5.0-0.012
- Mounting hole pitch: 31.0±0.1
- Motor body height: 42.0MAX
- Mounting hole depth: 4-M3 DEPTH 4.5MIN
- Harwin Connector length: 1000±10

Labels:

- Black Housing
- Harwin Connector 2.54mm 4-PIN

CONNECTIONS

Wiring diagram showing the connections for the motor:

- BLK (Black) wire connected to the top terminal.
- GRN (Green) wire connected to the bottom terminal.
- RED (Red) wire connected to the left terminal.
- BLU (Blue) wire connected to the right terminal.

17HS16-2004S1

技术规格书

标记 处数 分区 更改文件号 签名 日期

设计 标准化

审核

工艺 批准

阶段 标记 重量 比例

共 张 第 张

STEPPERONLINE
Motors & Electronics

www.OMC-StepperOnline.com

Table xx. Nema 17 Stepper Motor Specifications and Dimensions


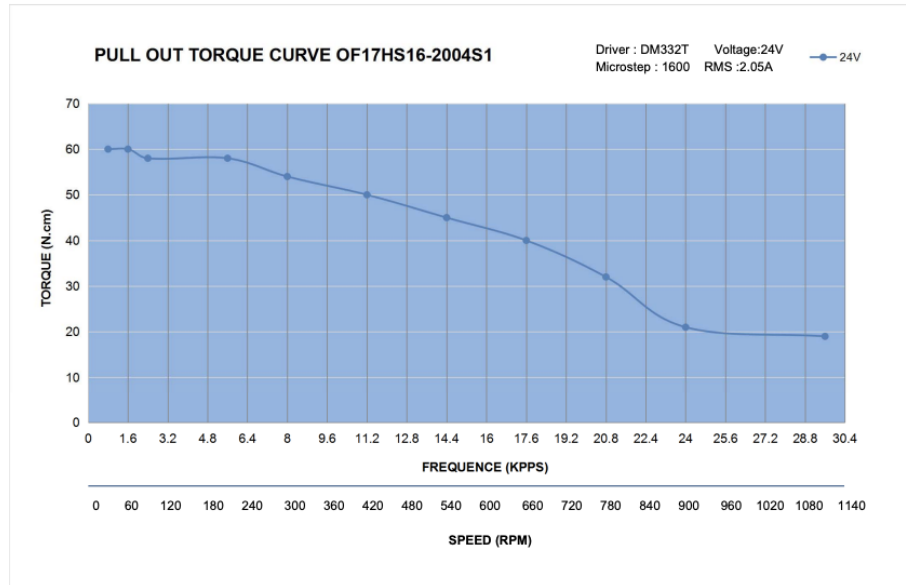


Figure xx. Nema 17 Stepper Motor Torque Speed Curve

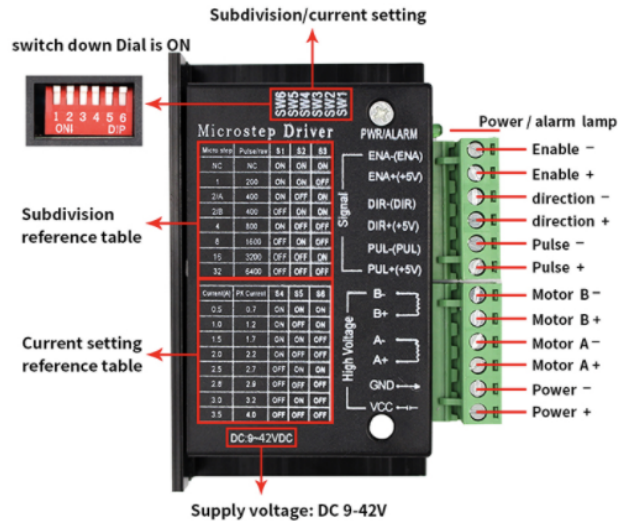

Feature:

This driver is an upgraded version of the TB6600

PWM chopper type bipolar stepper motor driver IC

1. 9V-42V DC power supply; H bridge bipolar constant phase flow drive.
2. The maximum 4.0A of the eight kinds of output current.
3. The largest 32 subdivision of the 6 models are optional.
4. Input signal high speed photoelectric isolation.
5. Common-anode standard single pulse interface. Offline to maintain the function.
6. Built-in temperature protection and over current protection.
7. To provide energy-saving semi-automatic current lock function.
8. Semi closed enclosure can be adapted to a more stringent environment.
9. Only the clock pulse signal can be driven two-phase bipolar stepper motor to achieve low vibration, high efficiency work.
10. Can control 2 phase stepper motor forward and reverse rotation, With 1-2, W1 -2 , 2W1 -2, 4W1 -2 phase excitation mode.

IC parameter:

single chip bipolar sine microstep stepper motor driver

the new BiCD 0.13 nm process

up to 42V , resistance (a +) = 0.4

the forward and reverse rotation control

5 subdivision mode options (1/1, 1/2, 1/4, 1/8, 1/16, 1/32)

rated output: IOU = 3.5 A

output current: IOU = 4.0A (peak, in 100ms)

package: HZIP25 - 1.00F

input port internal pull-down resistor: 100 K

alarm output pin current: Ialert = 1mA

monitoring output pin (MO): Imo = 1mA

with reset and enable pin, with standby function

Break through the traditional, single power supply

Undervoltage protection, built-in (UVLO) circuit

built in overheating protection (TSD) circuit

built-in overcurrent detection (ISD), circuit

Package Included:

1 x TB6600 stepper motor driver

Figure xx. Usongshine Stepper Motor Driver Specifications

Parameter

- Input: AC110V/220V 50/60Hz
- Output Voltage : DC 12V
- Output Current: 30A max
- Output Wattage: 360W max
- Fix Screw Hole Diameter: 2.5mm (0.1inch)
- Working temperature: -10 to 50 degree Celsius
- Storage temperature: -20 to 60 degree Celsius
- Environmental humidity: 10-95%
- Material: Metal, Electronic Parts
- Safety Compliance: CCC/ FCC / CE

Connection instruction

- L: Live wire
- N: Negative wire
- +V: DC power output "+"
- -V: DC power output "-"
- +V ADJ: Adjust the output voltage (10%)

Kindly note

1. High Voltage inside, do not remove the cover.
2. 110V/220V must be selected by switch before using to avoid damaging. Please change the switch to 110V for USA.
3. It comes without installation instruction, wiring cable, on/off switch and screws. Professional Installation of qualified electrician is highly recommended.

Package included

- 1 x 12V 30A Power Supply Switch

Figure xx. ALITOVE AC 110V/220V to DC 12V 30A 360W Universal Regulated Switching Power Supply Product Specifications

Code Written


(TBD)

Detailed Analysis

Lead Screw Analysis

The purpose of this static analysis was to determine the maximum linear force that our stepper motor coupled with our lead screw could produce. Some assumptions that were made was that the maximum torque of the Nema-17 we acquired, based on the specification sheet, was 0.45 Nm. Another assumption that was made was that the dry friction coefficient between the external threads of screw and the internal threads of the hex nut was 0.20. Therefore, the impending motion of the screw as it is supporting a load can be modeled as the 2D free body diagram seen in figure (). Here the green slope represents the external threads of the screw and the black outlined box represents the internal threads of the hex nut. The external threads of the screw are unwrapped to allow them to be modeled like this and therefore length of the base of this slope is equal to the circumference of the screw. The height of the slope represents another important

screw dimension which is the screw pitch. Screw pitch is the distance between the threads of a screw and can be found by taking the inverse of the threads per inch. The screw used for the syringe pump system has single start threads which means the screw lead, which is the linear distance travelled in one revolution by the screw is equal to the pitch of the screw. The particular screw used has 20 threads per inch and has right hand threads. Therefore, the lead and pitch can easily be calculated. Another dimension of importance is the mean diameter, or the pitch diameter, of the screw which can be found using a reference table since all screws made adhere to certain manufacturing standards that are based on their class. With all of this information the sum of the forces for the free body diagram can be solved for as well as the maximum linear force produced by the lead screw actuator.

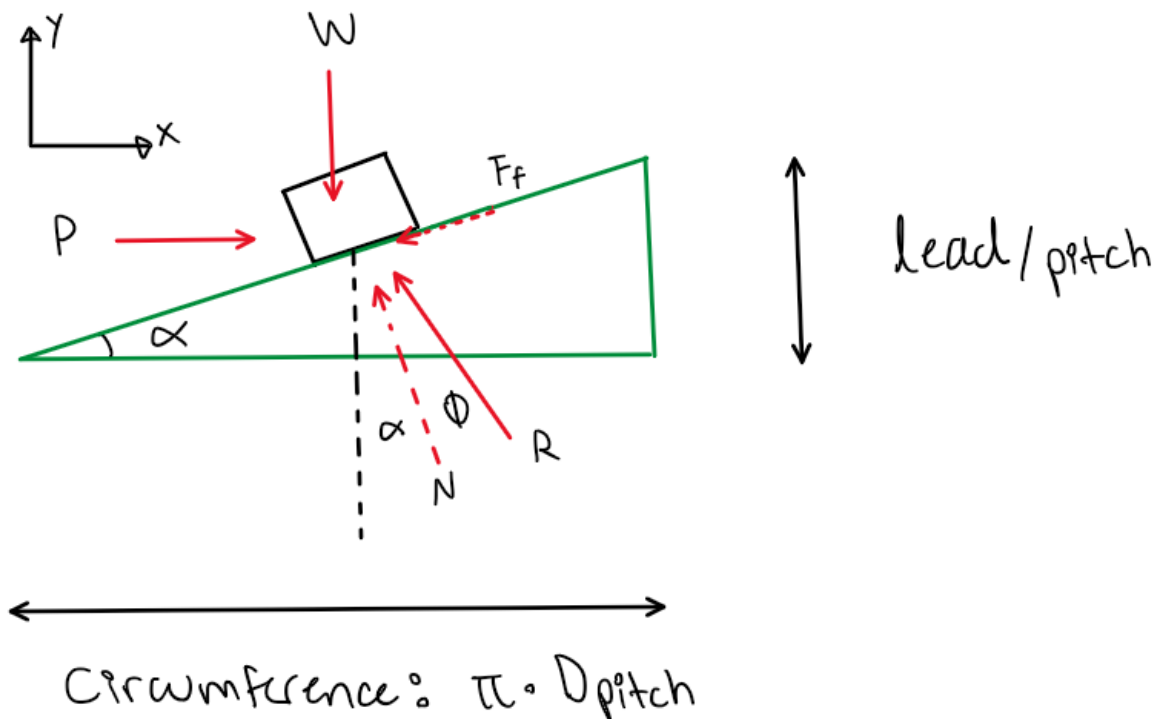

(Add equations here)

The results that were found during this lead screw analysis was that the maximum linear force provided by the lead screw mechanism was 593.3 N. This result is important because it gives the maximum baseline for the linear force produced by the linear actuator.

(Add references)

Linear Force Required Analysis

The purpose of this analysis was to characterize the forces that would be required during the operation of the syringe pump system. This analysis was done using Poiseuille's Law for Laminar Flow which states that the driving force for the flow of a liquid inside of a tube is the pressure difference between each end of the tube. Some assumptions that were made to perform this analysis were that the flow inside the syringe was completely laminar and that the friction from inside of the syringe was neglected. Other assumptions that were made were that the pressure at the tip of the syringe was at atmospheric pressure and that the flow rate was set at 2 mL/min. Also, water at 20 celsius was used as the liquid inside of the syringe to determine the fluid's viscosity. Next, the only remaining step was to measure with digital calipers the inner diameter as well as the length of each syringe used for this analysis. Now the only variable left to solve for was the linear force, F , that pushes the plunger of the

(add equations)

(add results)

(add references)

Budget

Name	Quantity	Cost (per quantity)	Cost (\$)
Stepper Motor	2	12.99	25.98
Linear Coupler (4 pc)	2	6.66	13.32
Ball Bearing Bushings (4 pc)	2	4.245	8.49
8 mm Linear Rods (2 pc)	1	10.89	10.89
Fully Threaded Rod	1	13.76	13.76
Stepper Motor Driver	2	8.79	17.58
Bluetooth Transiever	1	8.39	8.39
M3 0.5x14mm Flathead Screws	1	4.57	4.57
Nextion Touchscreen	1	112.3	112.3
12V 30A Power Supply	1	27.99	27.99
Tubing		0	0
3D printing filiment		0	0
3 Wire power cord	1	17.25	17.25
File	1	6.45	6.45
8 mm Linear Rods (2 pc)	2	8.99	17.98
Fully Threaded Rod	1	12.98	12.98
Servo Motor (4 pc)	1	23.69	23.69
5V 5A Power Supply	1	10.76	10.76
3 Wire power cord	1	11.31	11.31
Digital Caliper	1	10.99	10.99
Stylus Pen	1	8.81	8.81
Total			363.49
Remaining			636.51

Table XX. Budget (to date)

Project Management

Task Distribution

Intermediate Milestones

Risk Reduction Efforts

